

# SUNTECH


## Tango M2

www.SunTechMed.com Blog.SunTechMed.com Sales@SunTechMed.com part #82-0112-00 Rev. D

### Single-Patient Use Proper Cuff Placement Guide


#### Step 1

Place the microphone into the microphone pad as shown. The adhesive surface will keep the microphone inside the microphone pad.

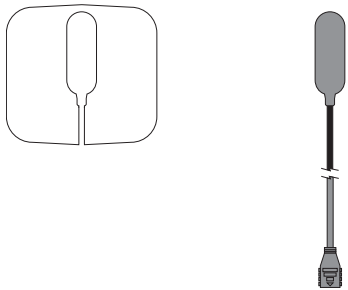


#### Step 2

Peel off the protective covering on the microphone pad as shown below.




#### Step 3

Microphone placement is essential to the performance of the Tango M2. Place the microphone over the brachial artery, in between the bicep and tricep muscles (approximately the width of 2 fingers above the elbow crease).

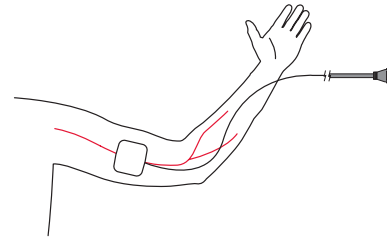


#### Step 4

Choose the appropriately-sized SunTech disposable cuff. The cuff has range markers on both the inside and outside to ensure proper sizing.

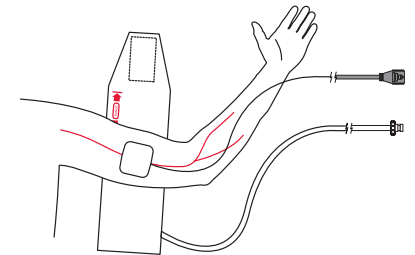


#### Step 5

Wrap the cuff securely around the arm. The artery marker should be over the brachial artery as shown below.

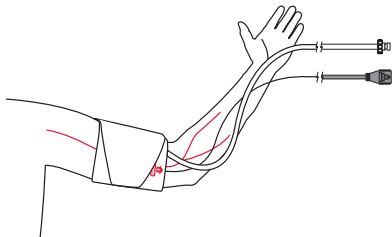


#### Step 6

Insert the microphone cable into the connector as shown below. The connectors can be inserted in any orientation. An audible click will be heard when a secure connection is made.

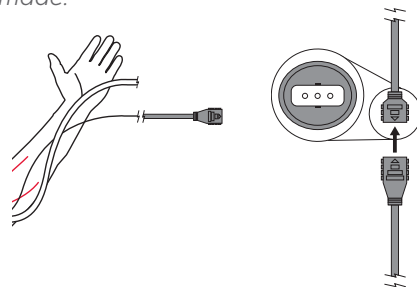

#### Step 7

Connect the cuff hose to the patient cable connector of the Tango M2 patient cable as shown below.

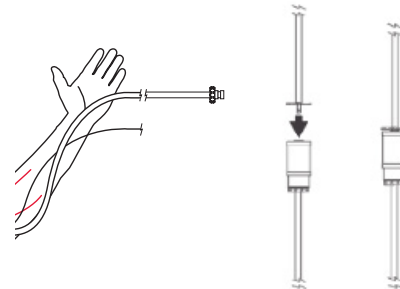

#### Step 8

Use the wrist straps provided with the Tango M2 system to secure both the patient cable and the microphone cable to the patient's wrist as shown below.

